



Advanced Test Equipment Rentals
www.atecorp.com 800-404-ATEC (2832)

EZCT-2000C

current transformer test set



Vanguard Instruments Company, Inc.
www.vanguard-instruments.com



EZCT-2000C

current transformer test set


Product Overview

The EZCT-2000C is Vanguard's third-generation micro-processor-based current transformer test set. Designed specifically for CT testing, the EZCT-2000C has the following outstanding features that can greatly increase productivity and save time during the commissioning stage:

- Performs CT excitation, current-ratio, polarity, and phase angle tests
- Measures insulation resistance and winding resistance of the CT secondary windings
- Measures the CT's load burden
- Standalone or computer-controlled via USB or Bluetooth wireless interface

The EZCT-2000C's test leads can be connected to all the CT output terminals, and the complete CT test can be performed automatically without any operator intervention.

EZCT-2000C connections

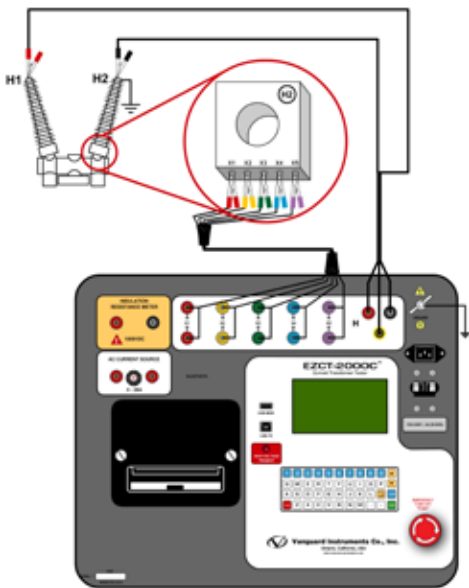

Excitation Test

The CT excitation test is performed using the ANSI/IEEE C57.13.1 test method. Test voltage ranges from 50, 300, 500, 1200 and 2000 Vac can be selected for the excitation test. The test voltage is raised and lowered automatically by the EZCT-2000C. The excitation test voltage and current data is collected and stored in the unit's internal memory. Knee point voltages (ANSI 10/50, IEC 60044, IEEE-30, IEEE-45) are calculated and printed on the test report. All of the test leads can be connected to the CT output terminals (X1, X2, X3, X4 and X5), and there is no lead switching required during testing. This convenient arrangement allows for testing any of the 10 possible combinations of X1 to X5. Up to 10 excitation tests can be stored in one record. Once the test is completed, the test report and CT excitation curves can be printed on the built-in thermal printer.

CT Winding Insulation Resistance Test Feature

The EZCT-2000C offers an IR test feature that can also measure the insulation resistance of the CT's secondary winding using a test voltage up to 1000 Vdc. The DC winding resistance reading range is from 2 to 500 Mega-ohms. The insulation resistance test results are displayed and printed on the report.

Ratio and Polarity Tests

The CT current-ratio is determined using the ANSI/IEEE C57.12.90 measurement method. A test voltage is applied on any two terminals (X1 to X5) of the CT, and the induced voltage is measured through the H1 and H2 terminals of the CT. The CT current-ratio is displayed and also stored in memory. The current-ratio is measured from 0.8 to 5,000. The CT winding polarity is displayed as a "+" sign (in-phase) or a "-" sign (out-of-phase) and is annotated with the phase angle in degrees. The CT current ratio error and phase displacement is also calculated based on the CT burden (or rated power) and rated current.

Demagnetization

The EZCT-2000C Plus automatically demagnetizes the CT under test when performing an excitation test.

Winding Resistance Test

The EZCT-2000C can measure the DC resistance of transformer windings from 100 micro-ohms to 10 ohms.

CT Burden Test

The EZCT-2000C can measure the CT's actual connected burden by injecting a 1A or 5A test current into the load. The CT burden measurements (Voltage, current, Cos ϕ , and burden impedance) are displayed on the screen and printed on the test report. This important test verifies the actual CT measured burden before putting the CT in service, thus avoiding any potential configuration conflicts.

Current Ratio and Phase Error Tables

As part of the tabulated test results, the EZCT-2000C can also print the current ratio and current phase error tables.


Current Source

The EZCT-2000C offers a programmable current source (0-20A, 0-15Vac) that can be used to verify CT loads. The on-time timer and output current are displayed on the LCD screen.

ordering information

Part No.	Description
9101-UC	110V EZCT-2000C, cables, and PC software
9102-UC	220V EZCT-2000C, cables, and PC software
9101-SC	EZCT-2000C shipping case
TP4-CS	TP4 thermal printer paper (24 rolls)

EZCT-2000C Controls & Indicators

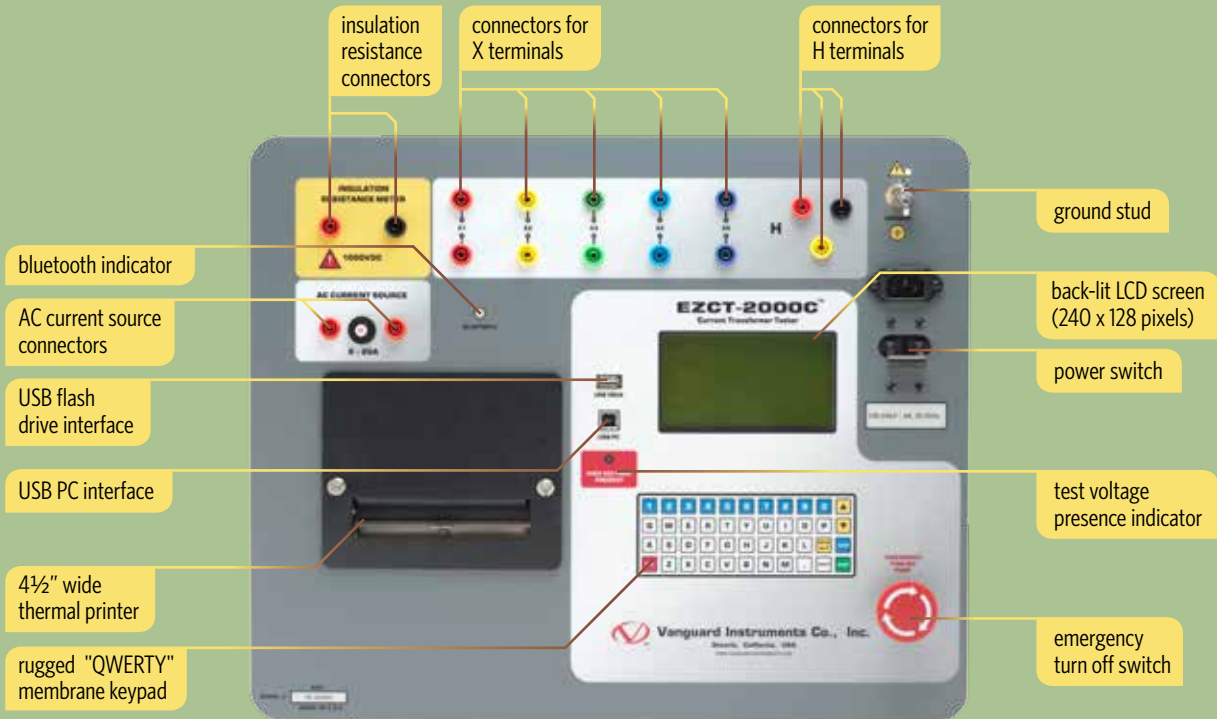

Test Record Header Information

Test record header information, including the company, substation name, circuit ID, manufacturer, mode, CT serial number, and the operator's name, can be stored with each record. In addition to the test record header, a 20-character test description for each test in the record (10 tests per record) can also be entered.

User Interface and Display

The EZCT-2000C features a back-lit LCD screen (240 x 128 pixels) that is clearly viewable in both bright sunlight and low-light levels. A "QWERTY"-style membrane keypad is used to enter test information and to control the unit's functions.

Computer Interface

The EZCT-2000C Plus can be used as a stand-alone unit or can be computer-controlled. It can be connected to a PC via the USB port or wirelessly via Bluetooth. In computer-controlled mode, using the included CT Analysis Software, test records can be downloaded from the unit's memory, or CT tests can be run from the PC. Test plans can also be created with the provided software. A test plan defines the various test parameters (test voltage, current range, nameplate ratios, etc.) and can be used to quickly perform tests. Additionally, tabulated test records are automatically exported to PDF, Excel, and XML formats for further analysis.

Built-in Thermal Printer

A built-in 4 1/2" wide thermal printer can print the current transformer test report and plot the excitation curves.

Internal Test Record Storage

The EZCT-2000C can store up to 140 test records in Flash EEPROM. Each record may contain up to 10 excitation curves, burden test reports, current ratio readings, and polarity and DC resistance readings. Test records can be recalled and printed on the built-in thermal printer. They can also be transferred to a PC using the USB port, wirelessly via Bluetooth, or via the USB Flash drive interface port.

External Data Storage

The EZCT-2000C features a USB Flash drive interface that makes it very convenient to store and transfer test records and test plans. By using a USB Flash drive, test records and test plans can be quickly transferred between a computer and the EZCT-2000C without the need to connect the unit to the computer.

Internal Test Plan Storage

The EZCT-2000C can store up to 128 CT test plans in Flash EEPROM. A test plan is comprised of the excitation test voltage, current range selection, CT nameplate ratios, and CT winding terminal combinations (X1 to X5) for each test and also includes the insulation test definition. Up to 10 test definitions can be stored per test plan. The ability to store test plans makes CT testing an extremely simple process. To perform a test, the EZCT-2000C is connected to the CT terminals and a test plan is selected to run.

Creating test plans for the EZCT-2000C is also a simple process. A test plan can be created using the EZCT-2000C's keypad or can be created on a PC (with provided software) and then downloaded to the EZCT-2000C via the USB port or Bluetooth. For added convenience, test plans can also be copied from a USB Flash drive to the EZCT-2000C via the USB Flash drive interface.

Android App

The EZCT-2000C can also be controlled wirelessly via the Bluetooth interface using the provided EZCT-2000 Android app. The full-featured EZCT-2000 app can be used to perform tests, create test plans, and transfer test records.

EZCT-2000C thermal printer output

RECORD NUMBER 1

CT EXCITATION TEST RESULTS

DATE: 01/07/15 TIME: 10:04:09

COMPANY:
STATION:
CIRCUIT:
MFR:
MODEL:
S/N:
COMMENTS:
OPERATOR:

TEST NUMBER: 1

TESTED TAP: X1-X2

TST NOTE:

TEST VTG RANGE: 300 V
TEST CUR RANGE: 2.0 A

WINDING RES: 212.1 m-OHMS

IEC 10/50 V_{kp}: 213.6 VOLTS
IEC 10/50 I_{kp}: 0.0858 AMPS

IEEE 30° V_{kp}: 198.0 VOLTS
IEEE 30° I_{kp}: 0.0736 AMPS

IEEE 45° V_{kp}: 165.7 VOLTS
IEEE 45° I_{kp}: 0.0586 AMPS


NAME PLATE RATIO: 1000:5
MEASURED RATIO: 199.97
PERCENT ERROR: 0.02 %
POLARITY: IN PHASE
PHASE ANGLE: + 0.04°
EXCITATION VTG: 98.2 VOLTS
EXCITATION CUR: 0.0388 AMPS

BURDEN	PERCENT RATED CURRENT (5.0 A)			
VA / COS φ	5%	10%	20%	40%
10.00 / 1.00	-0.09%	-0.09%	-0.04%	-0.04%
5.00 / 1.00	-0.03%	-0.03%	-0.03%	-0.03%
2.50 / 1.00	-0.02%	-0.02%	-0.02%	-0.02%
1.25 / 1.00	-0.02%	-0.02%	-0.02%	-0.02%
0.00 / 1.00	-0.02%	-0.02%	-0.02%	-0.02%

BURDEN	50%	100%	120%	200%
10.00 / 1.00	-0.04%	-0.04%	-0.04%	-0.03%
5.00 / 1.00	-0.03%	-0.03%	-0.03%	-0.02%
2.50 / 1.00	-0.02%	-0.02%	-0.02%	-0.02%
1.25 / 1.00	-0.02%	-0.02%	-0.02%	-0.02%
0.00 / 1.00	-0.02%	-0.01%	-0.01%	-0.01%

BURDEN	PERCENT RATED CURRENT (5.0 A)			
VA / COS φ	5%	10%	20%	40%
10.00 / 1.00	3.19*	3.20*	2.68	2.13
5.00 / 1.00	2.16*	2.15*	2.10	1.66
2.50 / 1.00	1.63*	1.63*	1.63*	1.35
1.25 / 1.00	1.38*	1.37*	1.37*	1.24
0.00 / 1.00	1.11*	1.11*	1.11*	1.08

BURDEN	50%	100%	120%	200%
10.00 / 1.00	1.98	1.51	1.44	1.23
5.00 / 1.00	1.52	1.19	1.10	0.95
2.50 / 1.00	1.28	1.00	0.94	0.76
1.25 / 1.00	1.12	0.89	0.84	0.68
0.00 / 1.00	1.00	0.77	0.73	0.61

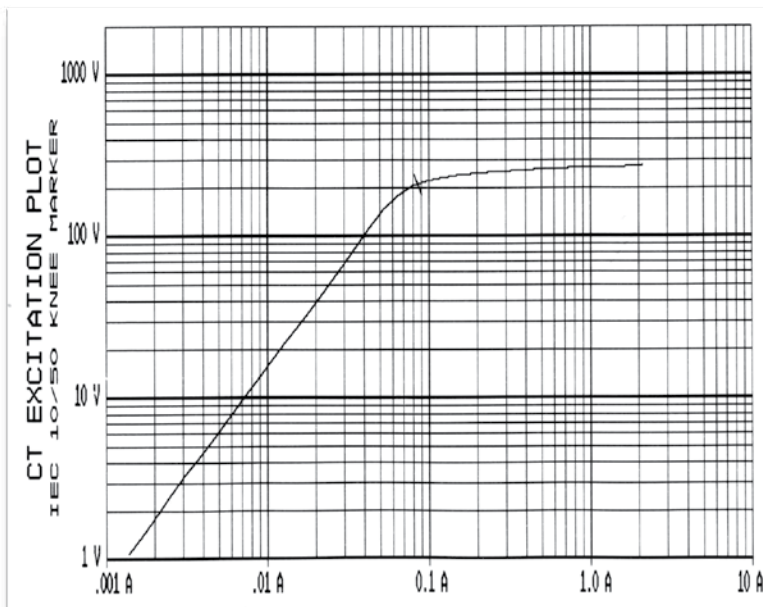

BURDEN TEST RESULTS

5 AMP BURDEN TEST

MEAS CURRENT: 4.979 A
MEAS VOLTAGE: 5.371 V, 359.2°
IMPEDANCE (Z): 1.079 OHMS

BURDEN: 26.959 VA
COS φ: 1.00

INSULATION RES TEST RESULTS



1000V INSULATION RES TEST

VOLTAGE: 997.7 V
CURRENT: 9.65 MICRO-AMPS
RESISTANCE: 101.27 MEG-OHMS


..... typical burden test results

..... typical insulation resistance test results

EZCT-2000C desktop printer output

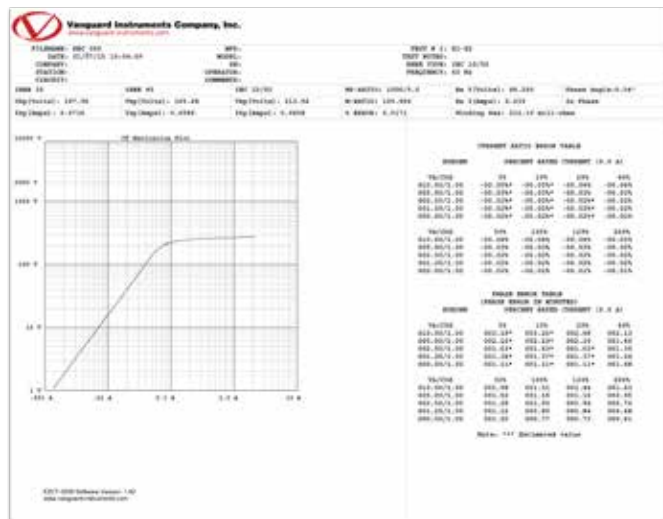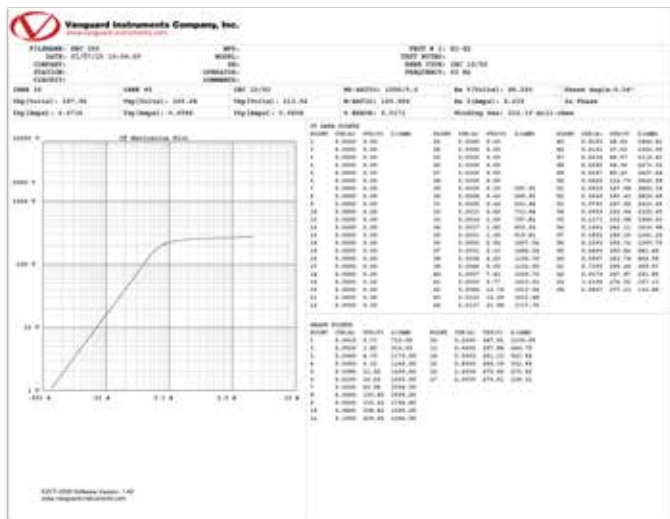

EZCT-2000C desktop printer output

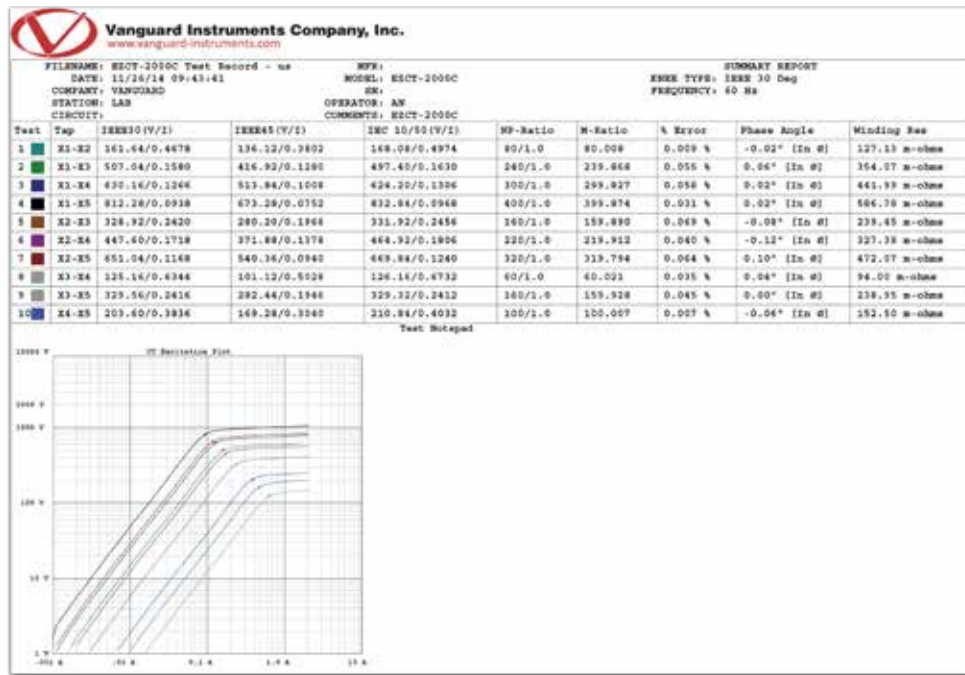

EZCT-2000C technical specifications

	physical specifications	Dimensions: 19"W x 13"H x 16"D (48.3 cm x 33cm x 40.1 cm) Weight: 73 lbs. (33.1 Kg)		input power	100 – 120 Vac or 200 – 240 Vac (factory pre-set), 50/60 Hz
	measuring method	ANSI/IEEE C57.12.90 and ANSI/IEEE C57.13.1 standards		current ratio range	0.8 – 999: ±0.1%, 1000 – 1999: ±0.3%, 2,000 – 5,000: ±1%
	output test voltages	0 – 50 Vac @ 10A max; 0 – 300 Vac @ 10A max; 0 – 500 Vac @ 5A max; 0 – 1200 Vac @ 1.2A max; 0 – 2000 Vac @ 1A max		current source	1 – 20A @ 0 – 15 Vac; displays test current and current on-time
	resistance reading range	100 micro-ohms – 30 ohms; accuracy: 2% of reading ±1 count, ±10 micro-ohms		insulation resistance test	2 M-ohms – 500 M-ohms; accuracy: 3% of reading; 500 – 1,000 Vdc test voltage
	voltage reading range	0 – 2,200 Vac accuracy: ±1.0% of reading, ±1 volt		current reading range	0 – 10 A, accuracy: ±1.0% of reading, ±0.02A
	display	back-lit LCD screen (240 x 128 pixels) viewable in bright sunlight and low-light levels		phase angle measurement	0 – 360 degrees accuracy: ±1.0 degree
	printer	built-in 4 1/2" wide thermal printer		computer interfaces	one USB port and bluetooth wireless interface
	pc software	Windows®-based CT analysis software is included with purchase price		external data storage	one USB flash drive interface port (flash drive not included)
	internal test record storage	stores 140 test records. Each test record may contain up to 10 sets of excitation, resistance and ratio data			
	internal test plan storage	stores 128 test plans. Each test plan can store 10 excitation test voltage and current settings		safety	designed to meet UL 61010A-1 and CAN/CSA C22.2 No. 1010.1-92 standards
	temperature	Operating: -10°C to +50°C (+15°F to +122°F) Storage: -30°C to +70°C (-22°F to +158°F)		humidity	90% RH @ 40°C (104°F) non-condensing
	cables	One 20-foot (6.10m) cable set (X1-X5), one 35-foot (10.69m) H cable set, current source cables, insulation test cables, power cord, ground cable, USB cable. A transportation case is included with the purchase price			
	altitude	2,000 m (6,562 ft) to full safety specifications		warranty	one year on parts and labor

NOTE: the above specifications are valid at nominal voltage and ambient temperature of +25°C (+77°F). Specifications are subject to change without notice.



Instruments designed and developed by the hearts and minds of utility electricians around the world.

Vanguard Instruments Company (VIC), was founded in 1991. Currently, our 28,000 square-foot facility houses Administration, Design & Engineering, and Manufacturing operations. From its inception, VIC's vision was, and is to develop and manufacture innovative test equipment for use in testing substation EHV circuit breakers and other electrical apparatus.

The first VIC product was a computerized circuit breaker analyzer, which was a resounding success. It became the forerunner of an entire series of circuit breaker test equipment. Since its beginning, VIC's product line has expanded to include microcomputer-based, precision micro-ohmmeters, single and three phase transformer winding turns-ratio testers, transformer winding-resistance meters, mega-ohm resistance meters, and a variety of other electrical utility maintenance support products.

VIC's performance-oriented products are well suited for the utility industry. They are rugged, reliable, accurate, user friendly, and most are computer controlled. Computer control, with innovative programming, provides many automated testing functions. VIC's instruments eliminate tedious and time-consuming operations, while providing fast, complex, test-result calculations. Errors are reduced and the need to memorize long sequences of procedural steps is eliminated. Every VIC instrument is competitively priced and is covered by a liberal warranty.



Vanguard Instruments Company, Inc.

1520 S. Hellman Avenue • Ontario, California 91761, USA
Phone 909-923-9390 • **Fax** 909-923-9391
www.vanguard-instruments.com

Revision A. May 28, 2015