



Advanced Test Equipment Corp.

www.atecorp.com 800-404-ATEC (2832)



ADT282

Dual-Channel Reference Thermometer Readout

ADT282 Dual-Channel Reference Thermometer Readout

-----User Manual

[Version: 2109V01]

Additel Corporation

STATEMENT

This user manual provides operating and safety instructions for the ADT282 Dual-Channel Reference Thermometer Readout. To ensure correct operation and safety, please follow the instructions in this manual. Additel Corporation reserves the right to change the contents and other information contained in this manual without notice.

Content

1. Introduction	6
1.1 General Introduction	6
1.2 Technical Specification.....	7
1.2.1 General Technical Specifications	7
1.2.2 Technical Specifications of Signal Measurement (Environment Temperature: 20±10°C, 1 year accuracy)	8
1.2.3 RTD Measurement	9
1.2.4 TC Measurement.....	11
1.3 Basic Structure	15
1.4 Power Supply.....	17
2. Display and functions.....	18
2.1 Main Display	18
2.2 Screen Lock and Unlock.....	19
3. Dual-Channel Thermometer Readout.....	20
3.1 TC Measurement	21
3.2 TC Measurement Setup.....	21
3.3 RTD Measurement.....	21
3.4 RTD Measurement Setup	22

3.5 Filter.....	22
3.6 Zeroing.....	23
3.7 Statistics	23
4. System Settings	24
4.1 Bluetooth.....	24
4.2 Power Management.....	24
4.2.1 Display Brightness.....	24
4.2.2 Battery Information	24
4.2.3 Auto Backlight Off	24
4.2.4 Auto Sleep	25
4.2.5 Auto power off.....	25
4.3 Service.....	25
4.3.1 Calibration	25
4.3.2 Maintenance	26
4.3.3 Factory Reset	26
4.4 Personalization	26
4.4.1 System Sound	26
4.4.2 Language	27
4.4.3 Date & Time.....	27
4.5 About Product	28
5. Data Management	28
6. APPS	28

6.1 Temperature Converter	28
6.2 Sensor Library	29
6.3 Data Logger	29
6.4 Temperature Unit	29
6.5 Temperature Differential.....	29

Safety Instructions

Warning:

To prevent the user from injury, please follow this user manual for use.

To prevent fire, electric shock or personal injury, please do as follows:

1. General:

- ◆ Please read the user manual before using the product;
- ◆ Before using the product, please check the appearance of the product to ensure there is no damage;
- ◆ Please refer to the operation steps in the manual when using the product;
- ◆ If the product is damaged or malfunctions, please do not use it and contact Additel;
- ◆ Never use the product in an explosive, steam or dust environment.

2. Electrical:

- ◆ Before using the product, please make sure that the power supply is connected correctly, and the installation is done properly.



Attention:

To prevent injury, please obey the instruction manual for use

To prevent damage, please do as follows:

- ◆ Do not use the instrument in a high vibration environment;
- ◆ If the product is abnormal, please stop using it and contact with Additel.

1. Introduction

1.1 General Introduction

ADT282 Reference Thermometer Readout delivers the best possible accuracies and features in the palm of your hand! With accuracy capabilities on par with laboratory grade thermometers, the ADT282 is capable of handling even your most critical measurements. This ultra-high precision readout features dual analog channels designed to facilitate comparison measurements and meet all your temperature measurement needs. The easy-to-use touchscreen makes navigating the well-designed menus a time saving and enjoyable experience. The Lemo style smart connectors help to ensure that your probe calibration information is never in question. The ADT282 Reference Thermometer Readout helps makes metrology simple and will quickly become your new go-to when reliable temperature measurements are necessary.

Contact us:

Additel Corporation

Tel: +1-714-998-6899

www.additel.com



1.2 Technical Specification

1.2.1 General Technical Specifications

Table 2 General technical Specifications

Display	5.0 inch 480*800TFT LCD capacitive screen
Dimensions	16.97" x 4.13" x 2.04" (177 mm x 105 mm x 52 mm)
Weight	1.5 lbs. (0.65 Kg)
Power Supply	6600mAh, 23.8Wh lithium battery, charging time 4~6 hours, battery pack can be charged independent. Battery life typically 16 hours
Environment	Specification guaranteed temperature range: (10~30)°C Working Temperature: (-10~50)°C Storage temperature: (-20~70)°C Humidity: 0 % ~ 95% RH, non-condensing Maximum altitude: 3000m
Warm-up Time	After 10 minutes of booting, specifications can be reached
Ports Protection Voltage	50Vmax

CE Certificate	TUV IEC61326, IEC61010
Rohs Compliance	Rohs II Directive 2011/65/EU, EN50581:2012
IP Protection Level	IP67, 1 meter drop test
Communication	Isolate USB-TYPE C (slave), Bluetooth BLE
Input Channels	CH1, CH2 analog channel, 6 pins smart Lemo ports for RTD probe; MINI-TC ports for TC probe
Measurement Display	Single channel, dual channel, differential (e.g., T1-T2)
Measuring Rates	<ul style="list-style-type: none"> ▪ CH1, CH2 analog channels alternately and cyclically measure ▪ RTD measuring rate: 1.6S/single channel, 1.6S/dual channel ▪ TC measuring rate: 0.8S/single channel, 0.8S/dual channel
Measurement Units	°C, °F, K
Statistics	Max, Min, Avg

1.2.2 Technical Specifications of Signal Measurement (Environment Temperature: 20±10°C, 1 year accuracy)

Table 3 Technical Specifications of signal measurement

Signal types	Range	Resolution	Accuracy
--------------	-------	------------	----------



RTD	0~400Ω	0.1mΩ	±0.5mΩ@ (0~20Ω) , ±25ppm@ (20~400Ω)
TC	-10~75mV	0.1uV	50ppmRDG+2uV
Internal CJC	NA	NA	±0.15°C (-10°C~50°C Guarantee specification)

Notes:

- When the environmental temperature is (-10~+10)°C and(30~50)°C,the temperature coefficient is:
 - RTD measurement: ±2ppmFS/°C.
 - TC measurement: ±5ppmFS/°C.
- RTD measurement excitation: 4 wires measurement, Constant current commutation, Excitation current: 1mA.

1.2.3 RTD Measurement

Table 4 RTD measurement (Environment temperature: 20±10°C)

RTD Types	Temperature(°C)		1 Year Accuracy(°C)
PT10(385)	-200~850	-200~200	0.014
		200~600	0.024
		600~850	0.033
PT25(385)	-200~850	-200~200	0.012
		200~600	0.024
		600~850	0.033

PT50(385)	-200~850	-200~200	0.012
		200~600	0.024
		600~850	0.033
PT100(385)	-200~850	-200~200	0.012
PT100(391)		200~600	0.024
PT100(3916)		600~850	0.033
PT100(3926)			
Cu10(427)	-200~260	-200~260	0.013
Cu50(428)	-50~150	-50~150	0.010
Cu100(428)	-50~150	-50~150	0.010
Ni100(617)	-60~180	-60~0	0.005
Ni100(618)		0~180	0.007
Ni120 (672)	-80~260	-80~260	0.007

Notes:

1. Conforms to the ITS90 international temperature standard, determined by the maximum tolerance of the RTD measurement, excluding the accuracy of the probe;



2. After connecting the probe, the combined accuracy can be calculated directly after the RSS (root-sum-square) of the probe accuracy and RTD measurement accuracy;
3. Additel provides short SPRT PT100 probes.

1.2.4 TC Measurement

Table 5 TC measurement (Environment temperature: 20±10°C)

TC Types	Temperature Range(°C)	0°C CJC compensation		
		1 Year Accuracy(°C)		
S	-50~1768	-50~0	0.51	0.53
		0~100	0.37	0.40
		100~1768	0.28	0.32
R	-50~1768	-50~0	0.54	0.56
		0~200	0.38	0.41
		200~1768	0.25	0.29
B	0~1820	200~300	1.01	1.02
		300~500	0.66	0.68
		500~800	0.41	0.44

		800~1820	0.28	0.32
K	-270~1372	-250~-200	0.48	0.50
		-200~-100	0.15	0.21
		-100~600	0.08	0.17
		600~1372	0.14	0.21
N	-270~1300	-250~-200	0.76	0.77
		-200~-100	0.22	0.27
		-100~1300	0.12	0.19
E	-270~1000	-250~-200	0.26	0.30
		-200~-100	0.10	0.18
		-100~700	0.06	0.16
		700~1000	0.08	0.17
J	-210~1200	-210~-100	0.13	0.20
		-100~700	0.06	0.16
		700~1200	0.10	0.18



T	-270~400	-250~-100	0.36	0.39
		-100~0	0.08	0.17
		0~400	0.05	0.16
C	0~2315	0~1000	0.16	0.22
		1000~1800	0.26	0.30
		1800~2315	0.42	0.45
D	0~2315	0~100	0.21	0.26
		100~1200	0.16	0.22
		1200~2000	0.27	0.31
		2000~2315	0.42	0.45
G	0~2315	50~100	0.60	0.62
		100~200	0.38	0.41
		200~400	0.24	0.28
		400~1500	0.16	0.22
		1500~2315	0.32	0.35

L	-200~900	-200~-100	0.07	0.17
		-100~400	0.06	0.16
		400~900	0.07	0.17
U	-200~600	-200~0	0.14	0.21
		0~600	0.05	0.16
LR	-200~800	-200~0	0.09	0.17
		0~800	0.06	0.16
A	0~2500	0~1200	0.20	0.25
		1200~2000	0.33	0.36
		2000~2500	0.48	0.50

Notes:

1. Conforms to the ITS90 international temperature standard, determined by the maximum tolerance of the TC mV measurement, excluding the accuracy of the probe;
2. After connecting the probe, the combined accuracy can be calculated directly after the RSS (root-sum-square) of the probe accuracy and RTD measurement accuracy;
3. Additel provides standard S-type TC probe with MINI-TC connector.

1.3 Basic Structure

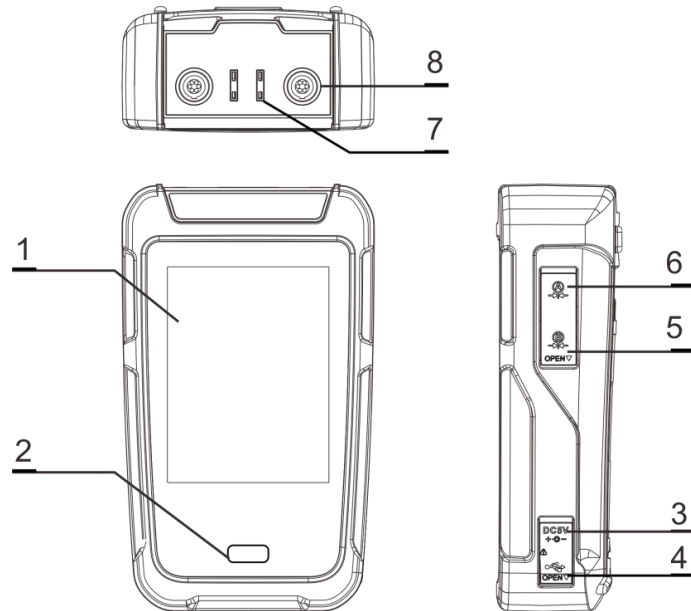


Figure 1 Basic Structure

Table 6 Basic structure list

No.	Part Name	Description
1	Display	Touchable display and capacitive screen
2	Power button	For switch on/off.
3	USB slave port	For USB connection.
4	Adapter port	For power supply.
5	Lemo style port B	Unusable yet, reserved for future development.
6	Lemo style port A	Unusable yet, reserved for future development.
7	Mini TC sockets	To connect mini-TC cable for TC measurement
8	RTD measurement sockets	To connect RTD probed for measurement

1.4 Power Supply

Smart lithium battery or external power adaptor power supply

- The smart lithium battery can be charged independently by using the power adaptor
- The power adapter quickly adapts to various countries power plugs



Figure2 Power adaptor and various countries power plugs

2. Display and functions

2.1 Main Display

The main operational interface is divided into three parts from top to bottom. The top section is the status bar, the middle section is the APPs list, and the bottom section is the main function navigation. (Figure 2-1)

1. The status bar includes time and date, battery status, lock screen status, Bluetooth and message control center.

Note: Click the status bar to enter the control center to view and control multi-function projects.

2. The APPs list shows all applications provided by the device, including data logging, pressure unit converter, temperature converter and sensor library.
3. The Main function navigation section provides access to three main functions at the bottom of the screen: Dual-Channel Thermometer Readout, Data Management and System Setup.

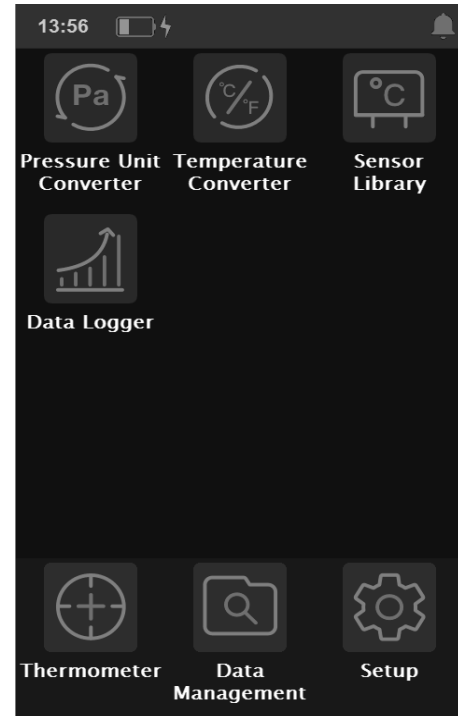




Figure 3 Main display



2.2 Screen Lock and Unlock



Lock screen: Click the status bar to enter the control center, you can click  to lock the current screen to avoid accidental operations. When the screen is locked, the icon  will be displayed in the status bar, and all operations are greyed out and prohibited on the screen.

Unlock screen: When the screen is locked, click the status bar to enter the control center to unlock the screen.

3. Dual-Channel Thermometer Readout

Dual-Channel Thermometer is one of the main functions of the device (figure 4). It can measure RTD and TC, both channels can be displayed at the same time, each channel measures a signal separately.

The measured signal value of the channel is displayed in the middle of the channel in real time, and the current signal type information is displayed on the upper left. Click the icon to switch the signal type. Click the menu icon  in the upper right corner to set the current channel in the pop-up menu. Click the zeroing icon  (when the channel supports it) to perform the zeroing operation on the current channel. If the signal type selected in the channel has multiple values for display (for example, when measuring TC, in addition to the temperature value, there are also the original mV signal value and the cold junction temperature value), then the channel will also display the main signal value. Other signal values are shown below.

The icons  and  in the upper right corner indicate whether the current temperature measurement channel is open and being displayed, click these icons to open or close the corresponding channel.

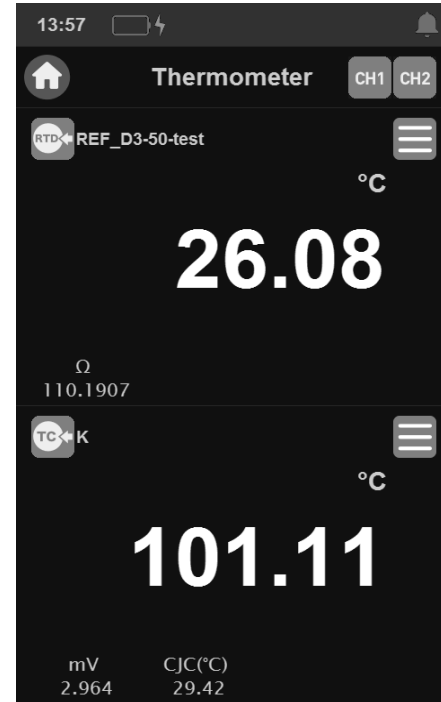




Figure 4 Thermometer



3.1 TC Measurement

There are 2 mini-TC sockets on the top of the unit, corresponding to two different channels. After connecting the TC to the device, click the type switch menu  or  of the corresponding temperature channel and select the TC to execute the TC measurement function.

3.2 TC Measurement Setup



Click “Setup” in the TC measurement menu to enter the TC setup. The following parameters can be set in this menu.

Table 7 TC Measurement Setup

Menu Selection	Effective value	Description
TC types	mV/TC sensors	Choose the TC sensors
Cold junction type	Internal/External/Custom	Choose the mode of cold junction. Built-in cold junction of device is used for Internal mode.
External cold junction compensation range	-80~300°C	Apply to external cold junction mode.
Temperature unit	K/°F/°C	Choose temperature unit
Resolution	0/0.1/0.01/0.001	Number of displayed decimal places

3.3 RTD Measurement

There are 2 Lemo style RTD measurement sockets on the top of the unit for connecting RTDs. After connecting the

RTD to the device, click the type switch menu  or  of the corresponding temperature channel and select the RTD to execute the RTD measurement function.

3.4 RTD Measurement Setup

Click “Setup” in the RTD measurement menu to enter the RTD setup. The following parameters can be set in this menu.

Table 8 RTD Measurement Setup

Menu Selection	Effective value	Description
RTD Types	Ω /RTD sensor types	Choose the RTD sensors
Temperature unit	K / °F/ °C	Choose temperature unit
Resolution	0/0.1/0.01/0.001	Number of displayed decimal places

3.5 Filter



The ADT282 Dual-Channel Thermometer Readout provides two filtering methods: first-order linear filtering and average filtering to meet the needs of different usage scenarios. Click the menu icon  of measurement channel to select the filter menu icon  in the pop-up menu and the filter setup interface will be displayed. (Table 9)

Table 9 Filter Setup





Menu Selection	Valid Value	Description
Enable/disable	Enable/disable	Set filter enable
Method	First-order filter/Average filter	Select filter method
Coefficient	0.01~1	Only available for first-order filter
Number of filter samples	1~100	Only available for average filter
Number of extremum pairs	0~10	Only available for average filter


3.6 Zeroing

mV and resistance signals provide short-circuit zeroing operation to eliminate zero-point drift. The allowable zeroing range is 1% FS.

3.7 Statistics

Click the menu icon  in the measurement channel and select the statistics menu in the pop-up menu, the maximum value Max, minimum value Min and average value Avg of the data will be displayed on the bottom of the channel display. Click the reset icon  on the top of the channel to reset the statistics.

4. System Settings

In the main screen of the device, click the system settings button  at the bottom right to enter the system settings interface. This page contains Bluetooth, power management, service, personalization, and about product.

4.1 Bluetooth

The calibrator has the Bluetooth communication function. Click the "Bluetooth" menu in the system setting interface to enter the Bluetooth communication setting interface. The Bluetooth communication setting interface provides the enable and disable of the Bluetooth communication function and the query function of the Bluetooth device name and physical address.

4.2 Power Management

4.2.1 Display Brightness

The LCD display brightness of the calibrator can be modified by adjusting the brightness progress bar.

4.2.2 Battery Information

This option displays the current battery connection status and information.

4.2.3 Auto Backlight Off

- ◆ If there is no button activity or communication command operations within the set time, the backlight brightness will be set to the lowest automatically;
- ◆ Backlight time can be set to: Never, 30 seconds, 1 minute, 5 minutes, 15 minutes, and 30 minutes.
- ◆ After the backlight is turned off, the first operational touch will restore the backlight to normal brightness, then, the subsequent touches will take effect normally.

4.2.4 Auto Sleep

- ◆ If there is no button activity or communication command operation within the set time, the backlight will be turned off automatically and start the auto sleep feature After the set time is up, the unit will go into the sleep status;
- ◆ The auto sleep timer can be set to: Never, 1 minute, 5 minutes, 15 minutes and 30 minutes.
- ◆ When using the power adapter for a power, the unit will never sleep;
- ◆ When the unit is running a data logging session, it will not sleep.
- ◆ If the backlight time is set to never, then the automatic sleep time setting is invalid.

4.2.5 Auto power off

- ◆ If there is no button activity or communication commands detected within the set time, the backlight will turn off, and the automatic shutdown timing will start after the start of auto sleep. After that time is up, the unit will be power off automatically.
- ◆ The auto power off timer can be set to: Never, 5 minutes, 15 minutes, 30 minutes, 1 hour and 2 hours.
- ◆ When using the power adapter for a power supply, it will not power off automatically;
- ◆ When the unit is running a data logging session, it will not power off automatically.
- ◆ If the backlight time is set to never, then the automatic power off time setting is invalid.

4.3 Service

4.3.1 Calibration

Click the “calibration” menu in the system setting interface and input the calibration password “123456” in the pop-up box to enter the system calibration interface. All the measurement signals in the device can be calibrated in the system calibration interface. The calibration process is as follows:

- 1) Select the item to be calibrated in the items list.

- 2) Use a high-precision standard device, after fully warming up, follow the calibration guide in the interface and click the "Start" button to start the calibration.
- 3) According to the reference calibration point provided on the system, select the appropriate standard value and enter it.
- 4) Click the "Finish" button to write the calibration data into the system to complete the calibration.
- 5) Click the "Restore" button at the bottom left of the calibration interface to restore the field calibration data of the device.

4.3.2 Maintenance

A password is required to access to this function. The factory default password is 123456.

- ◆ Maintenance records: The maintenance information can be viewed and edited.
- ◆ Calibration records: The calibration records can be viewed here.
- ◆ Operation information: The atmospheric pressure, motherboard and battery information.
- ◆ Error log: The error records can be viewed here.

4.3.3 Factory Reset

A password is required to enable this function. The factory default password is 123456.

- ◆ Restore the factory will not delete the system calibration data.

4.4 Personalization

4.4.1 System Sound

The volume of the Dual-channel Thermometer Readout can be modified by adjusting the volume progress bar. In addition, the prompt tone can also be configured. (Table 10)

Table 10 Sounds Settings

Menu Selection	Valid value	Description
Touch-tone	On/off	Set the touch-tone
Beep	On/off	Set the beep
Over-range beep	On/off	Set the over-range beep
Snapshot beep	On/off	Set the snapshot beep
Stable beep	On/off	Set the stable beep

4.4.2 Language

The device provides multi-languages which can be selected through this menu.

After the language is selected, the device needs to be rebooted for the change to take effect.

4.4.3 Date & Time

The data and time and format can be set as need, see Table 11.

Table 11 Data and time settings

Menu Selection	Valid value	Description
Date	2020-1-1 ~ 2048-12-31	Date setting
Time	00:00 ~ 23:59	Time setting
Date format	year-month-day / month-day-year / day-month-year	Date format setting
Delimiter	-, /, .	Delimiter setting
Time zone	UTC±00:00 ~ 12:00	Time zone setting

24 hours setting	Enable	Enable 24-hour display settings
------------------	--------	---------------------------------

4.5 About Product

Product information is read-only information, including basic information, version information and operating information:

- ◆ Basic Information: including product model, serial number and system version information.
- ◆ Module Information: including Bluetooth and temperature board version.

5. Data Management

- ◆ The data Management menu is classified and managed by different functional modules, and the data saved by each function is managed in the corresponding folder, which is convenient for users to review.
 - ◆ The types of data files that can be saved include: Snapshot and Data Logger.
 - ◆ Users can delete data files in batches.

6. APPs

6.1 Temperature Converter

The Dual-channel Thermometer Readout also provides a temperature converter application for various industrial RTDs, TCs, and custom sensor types, which can easily convert between temperature and electrical signals for different sensors.

6.2 Sensor Library

To meet the needs of user's sensor types, the unit provides a sensor library function. Users can define new sensor types according to their needs and set parameters in the sensors. The sensor library supports four types of custom sensors: ITS-90, CVD, Custom RTD and Standard TC.

6.3 Data Logger

The Thermometer Readout provides a data logging function. Users can set channels parameters for data logging. After editing the sampling settings, click the start icon again to start data logging. The settings are shown in Table 12.

Table 12 Data logger parameters settings

Subject	Valid value	Description
Logging interval	0.5~100	Data logging interval time
Logging points	2~100000	Number of logged data
Logging time	1~10000000	Logging Duration

6.4 Temperature Unit

Users can calculate the temperature in 3 different temperature units, °C, K and °F.

6.5 Temperature Differential

The Readout provides a Temperature differential function. Users can calculate the temperature differences between 2 channels with this function.



Additel Corporation

2900 Saturn Street #B

Brea, CA 92821 USA

Phone: 714-998-6899

Email: service@additel.com

website: www.additel.com